

Comparison of high-temperature conversion and equilibration methods for the determination of d31-palmitic acid oxidation in man using continuous-flow isotope ratio mass spectrometry

Valérie Sauvinet, Laure Gabert, Maud Alligier, Sylvie Normand, Hubert Roth, Martine Laville, Michel Désage

► **To cite this version:**

Valérie Sauvinet, Laure Gabert, Maud Alligier, Sylvie Normand, Hubert Roth, et al.. Comparison of high-temperature conversion and equilibration methods for the determination of d31-palmitic acid oxidation in man using continuous-flow isotope ratio mass spectrometry. *Rapid Communications in Mass Spectrometry*, Wiley, 2011, 25 (19), pp.2749-2759. 10.1002/rcm.5173 . hal-03254888

HAL Id: hal-03254888

<https://hal-univ-lyon1.archives-ouvertes.fr/hal-03254888>

Submitted on 9 Jun 2021

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Comparison of High Temperature Conversion and Equilibration methods for the determination of d₃₁-palmitic acid oxidation in Man using Continuous Flow Isotope Ratio Mass Spectrometry

Journal:	<i>Rapid Communications in Mass Spectrometry</i>
Manuscript ID:	RCM-11-0104.R1
Wiley - Manuscript type:	Special Issue Paper
Date Submitted by the Author:	n/a
Complete List of Authors:	Sauvinet, Valérie; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health; INSERM U1060, CarMeN Laboratory Gabert, Laure; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health; Hospices Civils de Lyon Alligier, Maud; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health; INSERM U1060, CarMeN Laboratory Normand, Sylvie; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health Roth, Hubert; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health Laville, Martine; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health; INSERM U1060, CarMeN Laboratory; Hospices Civils de Lyon Désage, Michel; Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health
Keywords:	deuterium, oxygen-18, continuous flow – isotope ratio mass spectrometry, equilibration, high temperature conversion
Abstract:	During nutritional interventions, the ingestion of d ₃₁ -palmitic acid and H ₂ ¹⁸ O allows assessment of dietary fatty acid oxidation from cumulative ² H recovery in urine and estimation of the total body water pool (TBW) from ¹⁸ O dilution. Continuous flow – isotope ratio mass spectrometry (CF-IRMS) coupled to either equilibration or high temperature conversion techniques (HTC) permits ² H and ¹⁸ O enrichment measurements in biological fluids. Thus it was of great interest to compare these methods applied to the determination of dietary fatty acid oxidation. Linearity, accuracy and correlation between CF-equilibration and CF-HTC were first checked using ² H- and ¹⁸ O- enriched water and urine samples. Urine samples from 14 subjects were then measured with both methods. ² H- and ¹⁸ O- raw data were normalised against calibration lines. The final aim was to study the impact of normalised raw results on physiological data (i.e. TBW and d ₃₁ -

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

	palmitate recovery).
	No significant difference was observed between $\delta^{18}\text{O}\text{‰}$ and $\delta^2\text{H}\text{‰}$ enrichment measurements depending on the analytical method used. Volumes of TBW calculated from $\delta^{18}\text{O}\text{‰}$ enrichments measured either with CF-equilibration or CF-HTC were not significantly different with respectively $45.2\pm 1.0\text{L}$ or $45.7\pm 1.0\text{L}$ (mean \pm sem, $p=0.09$). Palmitic acid oxidation results obtained from $\delta^2\text{H}\text{‰}$ enrichment measurements and TBW from CF-equilibration vs CF-HTC were not significantly different ($p\geq 0.26$) with respectively $16.2\pm 1.6\%$ vs $16.2\pm 1.1\%$ at 8h, $18.7\pm 2.0\%$ vs $17.6\pm 1.3\%$ at 12h and $21.7\pm 1.9\%$ vs $21.5\pm 1.3\%$ at 3 days post-dose (mean \pm sem).
	Thus, even if CF-HTC was preferred because it was more practical to carry out, both methods allow study of dietary lipid oxidation in man and generate similar results.

SCHOLARONE™
Manuscripts

Peer Review

1
2
3 **Comparison of High Temperature Conversion and Equilibration methods for the**
4 **determination of d₃₁-palmitic acid oxidation in Man using Continuous Flow Isotope**
5 **Ratio Mass Spectrometry**
6
7

8
9
10 **Valérie Sauvinet^{1,2*}, Laure Gabert^{1,4}, Maud Alligier^{1,2}, Sylvie Normand^{1,3}, Hubert**
11 **Roth^{1,5}, Martine Laville^{1,2,3,4} and Michel Désage^{1,3}**
12
13

14
15 ¹Lyon University, CRNH Rhône-Alpes and Center for European Nutrition, Safety and health,
16 F-69310 Pierre Bénite, France.

17
18 ²INSERM U1060, CarMen Laboratory, F-69921 Oullins, France

19
20 ³Lyon University, F-69310 Lyon Pierre Bénite, France

21
22 ⁴Hospices Civils de Lyon, F-69310 Pierre Bénite, France

23
24 ⁵INSERM U1055, CHU Grenoble, F-38043 Grenoble, France
25
26

27
28 **Correspondence to:* Valérie Sauvinet, Centre de Recherche en Nutrition Humaine Rhône-
29 Alpes (CRNH-RA) and CENS, Centre Hospitalier Lyon Sud, Centre de Biologie et Anatomie
30 Pathologie du Sud (CBAPS), Bât. 3D
31 165 chemin du Grand Revoyet, 69310 Pierre Bénite, France; phone number: +33 (0)4 78 86
32 29 81; fax number: +33 (0)4 78 86 66 54; valerie.sauvinet@chu-lyon.fr
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

ABSTRACT 250 words max

During nutritional interventions, the ingestion of d_{31} -palmitic acid and $H_2^{18}O$ allows assessment of dietary fatty acid oxidation from cumulative 2H recovery in urine and estimation of the total body water pool (TBW) from ^{18}O dilution. Continuous flow – isotope ratio mass spectrometry (CF-IRMS) coupled to either equilibration or high temperature conversion techniques (HTC) permits 2H and ^{18}O enrichment measurements in biological fluids. Thus it was of great interest to compare these methods applied to the determination of dietary fatty acid oxidation.

Linearity, accuracy and correlation between CF-equilibration and CF-HTC were first checked using 2H - and ^{18}O - enriched water and urine samples. Urine samples from 14 subjects were then measured with both methods. 2H - and ^{18}O - raw data were normalised against calibration lines. The final aim was to study the impact of normalised raw results on physiological data (*i.e.* TBW and d_{31} -palmitate recovery).

No significant difference was observed between $\delta^{18}O\text{‰}$ and $\delta^2H\text{‰}$ enrichment measurements depending on the analytical method used. Volumes of TBW calculated from $\delta^{18}O\text{‰}$ enrichments measured either with CF-equilibration or CF-HTC were not significantly different with respectively $45.2\pm 1.0L$ or $45.7\pm 1.0L$ (mean \pm sem, $p=0.09$). Palmitic acid oxidation results obtained from $\delta^2H\text{‰}$ enrichment measurements and TBW from CF-equilibration vs CF-HTC were not significantly different ($p\geq 0.26$) with respectively $16.2\pm 1.6\%$ vs $16.2\pm 1.1\%$ at 8h, $18.7\pm 2.0\%$ vs $17.6\pm 1.3\%$ at 12h and $21.7\pm 1.9\%$ vs $21.5\pm 1.3\%$ at 3 days post-dose (mean \pm sem).

Thus, even if CF-HTC was preferred because it was more practical to carry out, both methods allow study of dietary lipid oxidation in man and generate similar results.

Abbreviated title (up to 70 characters):**HTC or Equilibration for the determination of fatty acid oxidation****Key words (5 maxi): deuterium; oxygen-18; continuous flow – isotope ratio mass spectrometry; equilibration; high temperature conversion.**

INTRODUCTION

Stable isotopes are useful tools to study human metabolism in many situations.^[1] Body composition^[2] and total energy expenditure (TEE)^[3] can be measured by mass spectrometry using stable isotope labelled water, while the metabolism of proteins, lipids and carbohydrates can be measured using the appropriate labelled tracers (*e.g.* ²H-, ¹³C- or ¹⁵N- amino acids,^[4,5] ²H- or ¹³C- glucose,^[6,7] ²H- or ¹³C- fatty acids^[8]).

Assessing dietary fatty acid oxidation is of major importance during nutritional interventions. The conventional method using ¹³C-labelled fatty acids^[9] required measurement of ¹³C-enrichment in exhaled CO₂ and determination of total CO₂ production (V_{CO2}) by indirect calorimetry. Moreover an acetate correction factor was required due to ¹³C sequestration in the tricarboxylic (TCA) cycle.^[10] In 2001, Votruba *et al.*^[11] validated a simpler method using palmitic acid uniformly labelled with deuterium atoms (*ie* d₃₁-palmitic acid) and ¹⁸O-labelled water. During d₃₁-palmitic acid oxidation, the ²H label is removed from fatty acids during β-oxidation and TCA cycle. The deuterium atoms appear as ²H₂O which mixes with the body water pool, providing a cumulative record of fat oxidation, while ¹⁸O dilution gives the total body water (TBW) estimation. With this method, only urine samples need to be collected. V_{CO2} determination and acetate correction for the calculation of recovery are no longer needed and experimentation can be performed in free-living conditions, unlike the conventional method which requires that volunteers stay at the clinical investigation center for measuring respiratory gas exchanges (V_{CO2}) by indirect calorimetry.

Continuous flow – isotope ratio mass spectrometry (CF-IRMS) allows ²H and ¹⁸O enrichment measurements in biological fluids (plasma, saliva and urine). According to the method used, samples are converted into gaseous hydrogen, carbon dioxide or carbon monoxide carried by helium carrier gas inside the mass spectrometer source. Among commercially available devices, two methods are traditionally used: gas/liquid equilibration^[12-14] and carbon supported-high temperature conversion.^[15-17]

Principle of continuous flow gas/liquid equilibration method remains the same since the works of Epstein and Mayeda in 1953,^[18] Rolston *et al.* in 1976,^[19] or Horita *et al.* in 1989,^[20] using off-line devices: H₂O from biological fluids is equilibrated either with CO₂ gas or with H₂ gas in the presence of platinum to catalyze equilibration.^[13] Initially dedicated to water, CF-equilibration was also used in complex matrix like urine and plasma in our laboratory^[21-23] and other teams.^[13,24,25]

With carbon supported-high temperature conversion, the underlying principle is the Unterzaucher reaction.^[26] Water is converted in H₂ and CO in a glassy carbon reactor heated

1
2
3 at temperatures well in excess of 1000°C. H₂ and CO are then separated on a molecular sieve
4 column and introduced into the isotope ratio mass spectrometer source. Continuous flow high
5 temperature conversion method is widely used for ²H and ¹⁸O enrichment measurements in
6 biological fluids. In 2004, Richelle *et al.*^[27] applied this method to the determination of ²H
7 and ¹⁸O enrichments measurements in plasma samples of rats. High temperature conversion
8 was then presented as a promising tool to assess body composition and total energy
9 expenditure. In 2006, Ripoche *et al.*^[28] validated the accuracy of ²H and ¹⁸O enrichment
10 measurements in urine and plasma samples by comparison to classical dual-inlet methods. A
11 chromium tube was used for ²H reduction, and a glassy carbon reactor for ¹⁸O pyrolysis. More
12 recently, high temperature conversion of H₂O from urine and saliva was validated using a
13 glassy carbon reactor^[29].

14
15 Although equilibration and carbon supported-HTC techniques are well described in
16 the literature, these two methodologies have never been directly compared for the
17 measurement of ²H and ¹⁸O enrichments in urine samples. The principles are fundamentally
18 different. With the equilibration technique, the measurement is performed on the gas resulting
19 from the isotopic equilibrium between H₂O from the sample and the added equilibration gas.
20 With the HTC technique, results are produced directly from the liquid sample reaction in the
21 glassy carbon reactor. To facilitate the reading, in the following of this paper, carbon
22 supported-HTC was replaced by HTC and corresponds to the method of high temperature
23 conversion supported by a glassy carbon reactor.

24
25 This essay critically examines the two methods and their practicability with large
26 series of samples, which are current in nutritional intervention protocols in man. In this paper,
27 we first checked the agreement of results obtained from IAEA (International Atomic Energy
28 Agency) reference waters (SLAP2, GISP and VSMOW2) and from ²H- and ¹⁸O- enriched
29 water or urine samples using both methods. Then the results obtained with urine samples from
30 14 subjects, who participated in a nutritional intervention, were compared using either
31 continuous flow -equilibration or -HTC. The final aim was to study the impact of the raw
32 results (*i.e.* analytical results which are ²H and ¹⁸O normalised enrichments expressed in ‰)
33 on physiological data (*i.e.* TBW and d₃₁-palmitic acid recovery).

34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 **EXPERIMENTAL** 57 58 59 60

Samples

Preliminary tests

Linearity and accuracy tests between CF-equilibration and CF-HTC techniques for $\delta^2\text{H}\%$ and $\delta^{18}\text{O}\%$ enrichment measurements were performed using reference waters SLAP2 (Standard Light Antarctic Precipitation, $\delta^{18}\text{O} = -55.5\%$, $\delta^2\text{H} = -428.8\%$), GISP (Greenland Ice Sheet Precipitation, $\delta^{18}\text{O} = -24.8\%$, $\delta^2\text{H} = -189.5\%$) and VSMOW2 (Vienna Standard Mean Ocean Water, $\delta^{18}\text{O} = 0.0\%$, $\delta^2\text{H} = 0.0\%$) from the International Atomic Energy Agency (IAEA, Vienna, Austria), as well as ^2H - and ^{18}O -enriched waters. The correlation between equilibration- and HTC- data was evaluated with the analysis of ^2H - and ^{18}O - enriched water and urine samples. Eight water samples and nine urine samples were enriched with increasing quantities of $^2\text{H}_2\text{O}$ (99% enriched) and H_2^{18}O (10% enriched, Eurisotop, Saint Aubin, France). Dilutions were prepared gravimetrically. Final enrichments of water samples were previously determined by repetitive measurements against reference waters from IAEA and were used as expected values, ranging from $-8.2 \delta\%$ to $220.7 \delta\%$ for ^{18}O and from $-65.2 \delta\%$ to $1218.3 \delta\%$ for ^2H . For urine samples, the averaged enrichments measured in the present study ranged from $-2.7 \delta\%$ to $200.6 \delta\%$ for ^{18}O and from $-21.1 \delta\%$ to $1814.4 \delta\%$ for ^2H .

Protocol

Isotopic enrichments were measured in urine samples from 14 subjects. The subjects were fully informed of the purpose and potential risks of the experimental protocol. Individual informed written consents were obtained before the study which was approved by the Scientific Ethics Committee of Lyon (CPP Sud Est II). After collection of baseline urine samples, the subjects ingested $0.5\text{g}\cdot\text{kg}^{-1}$ of H_2^{18}O (10% enriched) to measure total body water. They then ingested a breakfast in which $20\text{mg}\cdot\text{kg}^{-1}$ of $[\text{d}_{31}]$ -palmitic acid (>98% enriched, *i.e.* 98% of palmitic acid molecules were labelled with 31 deuterium atoms, Eurisotop) were homogenized. Following ingestion of the meal, hourly urine samples were collected for 12h, and on days 1, 2 and 3 post-dose. Equilibration time in the body water pool for H_2^{18}O was taken at 4h and 5h post-dose. In order to determine the body water pool size, a dilution of the H_2^{18}O dose ingested was performed gravimetrically for each subject in Evian water (Dil.), in such a way as to obtain $\delta^{18}\text{O}\%$ enrichments similar to those in urine samples after tracer ingestion. Results from this sample determined the dilution factor of ^{18}O in the body, and consequently TBW. The determination of $[\text{d}_{31}]$ -palmitic acid oxidation rate required the collection of 13 urine samples. ^2H enrichment measurements were performed on all samples, whereas three urine samples and the diluted solution of the labelled water were analysed for

1
2
3 their ^{18}O content. No further details on clinical part of the protocol will be provided here,
4 insofar as the subject of this paper is to compare two analytical methods, and not to discuss
5 the results of the study which are to be published later.
6
7
8

9 10 *Sample processing*

11 Urine samples (2ml) were decolorized with dry black carbon (20mg), filtered (0.45 μm ,
12 cellulose acetate membrane, Macherey Nagel, Hoerd, France) and stored at -20°C until
13 analysis. Water samples were analysed without purification.
14
15
16
17

18 **Continuous Flow Equilibration**

19
20 Continuous flow equilibration analyses were performed using a Multiflow system connected
21 to an Isoprime IRMS (Isoprime Ltd, Cheadle, UK). 200 μL of standard water, ^2H and ^{18}O
22 enriched water or filtered urine sample were loaded in Labco Exetainer® vials with screw
23 caps and pierceable rubber septum (16.5mm, Labco Limited, Buckinghamshire, UK). A
24 platinum catalyst (Hokko coils, Elementar, Villeurbanne, France) was inserted into vials for
25 the hydrogen equilibration process to speed up the hydrogen isotope exchange reaction
26 between water and H_2 gas.^[30] Hokko coil catalysts were washed with deionised water and
27 conditioned at 80°C for 8 hours before use. Vials were placed in a temperature-controlled
28 rack ($40^\circ\text{C} \pm 0.1^\circ\text{C}$) offering 60 locations and filled either with CO_2/He (5%) or H_2/He (10%).
29 The equilibration times recommended by the manufacturer were 4h30 for CO_2 or 1h30 for H_2 .
30 Taking into account the autofilling time with equilibration gas (150sec /vial, at least 54 vials
31 in the rack), the real equilibration times were actually 4h30 for CO_2 and 2h15 for H_2 .
32
33 Equilibrated gas was then transferred from the vial's headspace to the sample loop (50 μL for
34 CO_2 or 100 μL for H_2) then on a molecular sieve GC column (90°C , 2.5m, 1/8 inch, 60-
35 80mesh) where all water vapour was separated. The dried gas was then allowed to pass from
36 the water trap (Nafion® membrane) to the isotope ratio mass spectrometer for analysis. The
37 sample peak was followed by one pulse of reference gas (H_2 grade 5.6 or CO_2 grade 5.5). The
38 $^2\text{H}/^1\text{H}$ ratios were corrected for the H_3^+ effect.^[31] Two batches of analyses were performed,
39 one for ^2H - and another for ^{18}O - enrichment measurements. To avoid refocusing the mass
40 spectrometer and changing the sample loop between each sequence, all samples from
41 preliminary tests and nutritional intervention were first analysed for their ^2H contents and then
42 for their ^{18}O content. Samples were prepared in triplicate for ^2H analyses, in duplicate for ^{18}O
43 analyses and were each injected three times. Even if no memory effect was observed using
44 equilibration method,^[32] urine samples were analysed in the ascending enrichment order. The
45 total analysis time for 20 samples including the autofilling with equilibration gas,
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 equilibration time and analyses, was 15h for ^2H enrichment measurements and 13h for ^{18}O
4 enrichment measurements. The total volume of purified urine required for the ^2H - and ^{18}O -
5 analysis of each sample was 1mL.
6
7
8

9 10 **Continuous Flow High Temperature Conversion**

11 High temperature conversion analyses were performed using a commercial device consisting
12 of a Thermo AS3000 liquid autosampler, a high-temperature conversion elemental analyser
13 (TCEA) coupled with a Delta Advantage isotope ratio mass spectrometer via a Conflow IV
14 Interface (Thermo Scientific, Bremen, Germany). According to the manufacturer design, the
15 reactor consisted of a glassy carbon tube (OD 12mm, ID 7mm, length 356mm) containing
16 carbon granulates (diameter $\geq 3\text{mm}$) above a quartz wool pad. This set was inserted in a
17 ceramic tube (OD 17mm, ID 13mm, length 470mm). A stainless steel injector sleeve (opening
18 $\sim 8\text{mm}$, length 60mm) was placed at the top of the glassy carbon tube. The following
19 conditions were used: reactor temperature 1420°C , GC column temperature 90°C and helium
20 flow from the top of the reactor 90 mL/min. Standard waters and filtered urine samples were
21 thawed and $300\mu\text{L}$ aliquots were transferred to a vial for autosampler with an insert (Agilent,
22 Massy, France). The insert was entirely filled with sample in the aim to reduce isotope
23 exchange in the sample container. Aliquots of $0.1\mu\text{L}$ were injected into the glassy carbon
24 reactor where water from samples was converted into H_2 and CO , which were then separated
25 on the molecular sieve GC column (0.6m , $\frac{1}{4}$ inch, 5A°). In order to keep optimal separation
26 conditions, GC column was heated to 300°C overnight every 2000 injections. Each analytical
27 run consisted of two pulses of the hydrogen reference gas (grade 5.6) followed by elution of
28 H_2 (retention time (RT) = 123sec) and CO (RT = 183sec) gases from the sample, and then
29 finally by two pulses of carbon monoxide reference gas (grade 4.7). After the elution of the
30 H_2 peak, a "peak jump" occurred at 150sec, allowing CO analysis: ion beams of m/z 28
31 (C^{16}O) and m/z 30 (C^{18}O) were then focused to specific Faraday cups by a rapid change in the
32 magnetic field strength. The $^2\text{H}/^1\text{H}$ ratios were corrected for the H_3^+ effect.^[31]
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49

50 Inter-samples memory effects have been reported for water analyses using the high
51 temperature conversion of water on glassy carbon. Precautions were taken to minimize this
52 well-documented effect:^[27,28, 32,33,34, 35] I) the sample was injected after 3 pull-ups, (II) the
53 needle of the $1\mu\text{L}$ syringe was left in the heated injector for 10sec after the injection, (III)
54 urine samples were analysed in ascending enrichment order and finally, (IV) for each sample,
55 five consecutive injections were done in a single run, and then the sample was injected once
56 in five consecutive runs. Only the last four runs were used for calculations. In these
57 conditions, the total analysis time for 20 samples was 16h for both isotopes enrichment
58
59
60

measurements. The total volume of purified urine required for the ^2H - and ^{18}O - analysis of each sample was $300\mu\text{L}$, each sample injection requiring only $0.1\mu\text{L}$.

Corrections, calibration and order of samples analysis

^2H and ^{18}O enrichments were expressed in $\delta\%$ vs VSMOW. Laboratory water (Evian®, Evian, France) was analysed at the beginning and the end of each sequence. Raw data obtained from these samples were used to calculate the drift value due to the long period of analysis. Using this value and the forecast function of the software Excel (pack Office 2002, Microsoft®), the drift-correction was applied to each sample of a same batch of analyses. Calibration was the same for the samples from preliminary tests and for those from the nutritional intervention. Three water standards from Iso-analytical Limited (Cheshire, UK; IA R053, $\delta^{18}\text{O} = -10.18\%$, $\delta^2\text{H} = -61.7\%$; IA R054, $\delta^{18}\text{O} = 0.56\%$, $\delta^2\text{H} = 4.93\%$ and IA R055, $\delta^{18}\text{O} = 108.63\%$, $\delta^2\text{H} = 843.43\%$ relative to VSMOW) were used to establish the calibration curve for normalisation of the values. For both techniques, the isotopic composition of enriched waters and urine samples was calculated from raw data using the linear regression equation obtained from known and measured values of these water standards. Concerning the order of samples analysis, for both techniques, ^2H - and ^{18}O - enriched waters, reference waters from IAEA and standard waters from preliminary tests were analysed in the ascending enrichment order. ^2H - and ^{18}O - enriched urine samples and samples from nutritional intervention were measured as following for both methods: laboratory water was first measured, then standard waters in the ascending enrichment order. Another laboratory water was injected to avoid memory effect on the following urine samples which were injected in the ascending enrichment order. Finally laboratory water was measured a last time for the drift correction.

Calculations

The oxidation rate of palmitic acid was inferred from the cumulative recovery of ^2H in total body water (TBW) according to Votruba *et al.*:^[11] TBW was determined using the ^{18}O isotope dilution method.^[2] First, the equation (1) allowed H_2^{18}O dilution space calculation from baseline and 4h or 5h urine samples, plus dilution of the ingested dose and Evian water which were analysed in the same batch.

$$N(\text{mol}) = \left(\frac{D_{\text{H}_2^{18}\text{O}} \times V_{\text{Dil}}}{MW_{\text{H}_2\text{O}} \times v_{\text{H}_2^{18}\text{O}}} \right) \times \left(\frac{\delta^{18}\text{O}_{\text{Dil}} - \delta^{18}\text{O}_{\text{Evian}}}{\delta^{18}\text{O}_{\text{T4or5h}} - \delta^{18}\text{O}_{\text{basal}}} \right) \quad (1)$$

1
2
3
4
5 N is the pool space in moles (*i.e.* the oxygen dilution space), $D_{H_2^{18}O}$ is the weight of labelled
6
7 water administered in g, V_{Dil} is the total amount of water (Evian + $H_2^{18}O$) used to dilute the
8
9 labelled water in g, $v_{H_2^{18}O}$ is the labelled water diluted for analysis in g, MW_{H_2O} is the
10
11 molecular weight of water in $g \cdot mol^{-1}$; and $\delta^{18}O$ is the enrichment in ‰ of the diluted labelled
12
13 water for analysis (Dil.), dilution water (Evian), post-dose sample (T4 or 5h, the maximum
14
15 $\delta^{18}O$ ‰ enrichment was used for calculations), and pre-dose baseline (basal). Next, using the
16
17 equation (2), TBW was deduced from the dilution space of ^{18}O (N) after adjusting it by a
18
19 factor of 1.007. Indeed, it is established that the dilution space of ^{18}O is 1.007% greater than
20
21 the water space.^[2]

$$22$$

$$23$$

$$24 \quad TBW(L) = \frac{N \times MW_{H_2O}}{1.007 \times 1000} \quad (2)$$

$$25$$

$$26$$

27 Finally, recovery of deuterium from palmitic acid oxidation was calculated as indicated by
28
29 equation (3)

$$30$$

$$31 \quad \% Recovery = 100 \times \frac{(TBW \times 2 \times \Delta\delta \times R_{STD} / 1000)}{(D \times P \times n / MW \times 100)} \quad (3)$$

$$32$$

$$33$$

34 $\Delta\delta$ was the urine δ^2H in excess compare to basal and was expressed in ‰ (“basal” being 2H ‰
35
36 enrichment from urine before the ingestion of the tracer) R_{STD} was the $^2H/^1H$ ratio of SMOW,
37
38 D was the amount of ingested d_{31} -palmitic acid in g, P was the 2H isotope atom‰ of d_{31} -
39
40 palmitic acid, n was the number of labelled atoms per molecule, and MW was the molecular
41
42 weight of d_{31} -palmitic acid in $g \cdot mol^{-1}$.

43 44 45 **Statistical analysis**

46 Regarding the raw data from the 14 subjects, a Bland and Altman^[36] test was used to evaluate
47
48 differences between $\delta^{18}O$ enrichments measured using either high temperature conversion or
49
50 equilibration. A mixed model was used for δ^2H enrichment comparison. Significant
51
52 differences between TBW obtained from $\delta^{18}O$ measurements with equilibration or HTC
53
54 techniques were tested using a paired Student test. Cumulative recoveries of d_{31} -palmitic acid
55
56 obtained from δ^2H and $\delta^{18}O$ measurements with equilibration or HTC techniques were tested
57
58 using a paired Student test and finally, a Bland and Altman test was used to evaluate
59
60 differences between recoveries of d_{31} -palmitic acid 3 days after the ingestion of the tracer
according to the analytical method used. The analyses were performed with Statview (Abacus

1
2
3 Concepts, Inc., Berkeley, CA) or Stata 11 (Stata Corp LP, Texas, US)), and values are the
4 mean \pm sem, with $p < 0.05$ considered statistically significant.
5
6

7 8 **RESULTS – DISCUSSION**

9 10 11 **Preliminary tests**

12 Before analysing the samples from the nutritional intervention, the linearity of ^2H - and ^{18}O -
13 enrichment measurements, *i.e.* correlation between measured and expected enrichments, and
14 accuracy of both methods were checked by analysing enriched water samples. Then the
15 correlation between equilibration- and HTC- data was evaluated with the analysis of enriched
16 water and urine samples. Table 1 shows ^{18}O - and ^2H -enrichments measured either by CF-
17 equilibration or CF-HTC, in reference waters from IAEA (SLAP2, GISP and VSMOW2),
18 enriched water samples, and enriched urine samples. These measured values were normalised
19 against calibration points from Iso-analytical Limited (IA R053, IA R054 and IA R055).
20 Linearity, accuracy and correlation results were obtained from these data.
21
22
23
24
25
26
27
28
29
30

31 *Linearity*

32 Table 2 shows regression parameters calculated from theoretical enrichments against
33 measured values in enriched waters, both expressed in ‰. The coefficients of determination
34 were greater than or equal to 0.9999. Linearity of ^2H - and ^{18}O - enrichment measurements was
35 as satisfying for equilibration measurements as for HTC measurements and the same is true
36 for ^2H - and ^{18}O -measurements. Data were comparable with those published elsewhere.^[12,13,29]
37
38
39
40
41
42

43 *Accuracy*

44 Table 3 shows individual accuracy data calculated from ^2H and ^{18}O enrichment measurements
45 of enriched waters presented in Table 1. The means of accuracy results obtained for the whole
46 range of ^{18}O - enrichments were $-0.54 \pm 0.30\%$ and $-0.39 \pm 0.34\%$ when samples were measured
47 by CF-equilibration or CF-HTC respectively. For the whole range of ^2H - enrichments, the
48 means of accuracy results were respectively $-1.00 \pm 3.33\%$ and $-1.52 \pm 3.39\%$ when samples
49 were measured by CF-equilibration or CF-HTC respectively. The difference from the
50 expected value was smaller for ^{18}O enrichment measurements and remained under 1.80%.
51 Results were less favourable for ^2H enrichment measurements and reached 8.51%. Accuracy
52 results were similar between both methods (t-test, $p > 0.1$). They corresponded to the level of
53 accuracy reported in the literature^[27,28] and remained acceptable.
54
55
56
57
58
59
60

Correlation between equilibration- and HTC-CF-IRMS

Table 4 presents the correlation parameters between data obtained with the equilibration technique and the HTC technique, for $\delta^{18}\text{O}\%$ measurements and for $\delta^2\text{H}\%$ measurements in water samples and in urine samples of increasing enrichments. Expected enrichments were in a range of $-55.5\ \delta\%$ to $220.7\ \delta\%$ for ^{18}O and of $-428.0\ \delta\%$ to $1218.3\ \delta\%$ for ^2H in water samples (including IAEA reference waters). For urine samples, averaged enrichments measured in this study ranged from $-2.7\delta\%$ to $200.6\delta\%$ for ^{18}O and from -21.1 to $1814.4\delta\%$ for ^2H . The slopes were respectively 1.0030 and 1.0049 for ^2H - and ^{18}O - measurements in water samples, and respectively 0.9993 and 0.9948 for ^2H - and ^{18}O - measurements in urine samples. The coefficients of correlation R were 1.0000 in all cases. Thus, there is excellent agreement between the two introduction systems and this is true whatever the isotope (^2H or ^{18}O) or sample nature. It should be noted however that the intercepts were different according to the sample type (water or purified urine). When measurements were performed on water samples, the intercepts were respectively 0.0558 and -1.4604 for ^2H - and ^{18}O - measurements. With urine samples, the intercepts were 0.7228 for ^{18}O and 8.4954 for ^2H -measurements, suggesting a bias between the 2 methods. In the case of measurements by HTC, the entire sample is injected into the reactor. Indeed, one fundamental difference between equilibration and HTC is that the equilibration reaction takes place between the equilibration gas and the H_2O molecules of the samples, whereas HTC measurements involve a bulk analysis of the sample including water. Some authors used a larger amount of black carbon to purify urine samples.^[28] An insufficient purification of urine samples may explain this result. This could be a serious drawback if the accurate isotopic contents were needed. But in metabolic studies performed in the field of nutrition, the measured enrichments in biological samples are always compared to a basal value measured in a sample of same type before the tracer ingestion. This is true for the calculation of Total Body Water,^[2] Total Energy Expenditure,^[3] or Dietary Fat Oxidation,^[11] using ^2H - and/or ^{18}O - labelled water.

Analytical results

We shall now look at the analytical results from the urine samples of the 14 subjects who took part in the protocol. Analytical results were the normalised $\delta^{18}\text{O}\%$ - and $\delta^2\text{H}\%$ - enrichments measured by CF-IRMS coupled either to equilibration or HTC. The set of water standards used to normalise the data was included in each sample batch. The equation of the calibration curve was therefore established for each series of analyses, in order to compensate for any changes that might occur during the analytical process (*e.g.* temperature variation during equilibration,^[11] reactor lifetime with HTC).

$\delta^{18}\text{O}\text{‰}$ enrichment measurements

Figure 1(A) shows the average of $\delta^{18}\text{O}\text{‰}$ enrichments obtained in the urine samples at baseline, before the ingestion of H_2^{18}O by subjects and at 4h and 5h post-dose. $\delta^{18}\text{O}\text{‰}$ enrichments were also measured in the dilution of the labelled water dose (Dil.) ingested by subjects, and in the water used to dilute this dose (Evian). All these measurements enter in the calculation of the volume of TBW using equations (1) and (2). $\delta^{18}\text{O}\text{‰}$ enrichments at baseline were found at $-3.8 \pm 0.3\text{‰}$ and $-4.0 \pm 0.3\text{‰}$ (mean \pm sem) using respectively equilibration or HTC. Equilibration of labelled water in urine was reached after 4 or 5h depending on the subjects, and was found at $41.4 \pm 1.3\text{‰}$ and $41.2 \pm 1.3\text{‰}$ using equilibration or HTC respectively for the analyses. The dispersion of $\delta^{18}\text{O}\text{‰}$ enrichment measurements, namely, the standard deviation of replicates injection, was greater with the equilibration technique compared with HTC. Standard deviations averaged $0.37 \pm 0.24\text{‰}$ for all the measurements, and were about 3 times higher than those obtained with thermal conversion elemental analysis ($0.14 \pm 0.20\text{‰}$). Nevertheless, for each sample from the 14 subjects, no significant difference was observed depending on the analytical method used (paired t-tests, $p > 0.11$). A Bland and Altman test (Fig.1(B)) that presents the differences between results from both methods in function of their respective average, showed a good agreement between both methods for $\delta^{18}\text{O}\text{‰}$ enrichment measurements with a mean bias of 0.12‰ and a confidence interval of differences between -3.51 and $+3.27\text{‰}$. Further purification of urine samples should reduce the bias between the two methods, including increasing the amount of black carbon. This step appears to be essential to obtain good quality of analyses using HTC.

$\delta^2\text{H}\text{‰}$ enrichment measurements

The evolution of deuterium enrichment in urines samples until 3 days after ingestion of d_{31} -palmitic acid is presented in Figure 2. $\delta^2\text{H}\text{‰}$ enrichment in urine continuously increased until the end of the test, sharply from 60 to 480min after ingestion of the deuterated fatty acid, and moderately after 480min. A plateau was reached during the last 2 days. As can be seen from Fig.2(A), the results for one subject show that the dispersion of $\delta^2\text{H}\text{‰}$ enrichment measurements was greater with the equilibration technique than with high temperature conversion. Standard deviations averaged $7.26 \pm 2.11\text{‰}$ and were about 16 times higher than those obtained with HTC technique ($0.45 \pm 0.23\text{‰}$). The fact that each sample vial was injected several times may explain this dispersion problem with equilibration method. Indeed, the repeated injections from a same vial result in a decrease of the signal amplitude. No more

1
2
3 than three injections are possible using H₂O/H₂ equilibration. Moreover, due to the device
4 configuration, the number of vial for each sample was limited to 3 in order to analyse all
5 samples from one subject (see Experimental part). Nevertheless, Fig.2(B) provides the results
6 for the 14 subjects and shows that the average values of deuterium enrichments in delta ‰
7 were homogeneous. The previous observation was confirmed by applying a mixed model
8 which did not show any significant differences between the two methods for δ²H‰
9 measurement (p=0.513). Using equilibration, results are dependent on the parameters
10 influencing the isotopic exchange process between liquid and gaseous phases, *i.e.* temperature
11 and catalyst efficiency. These two parameters are not easy to control. Due to the temperature-
12 dependent fractionation factor of hydrogen between liquid and gas phases, a temperature
13 variation of only 1°C during the equilibration process can cause a difference of 6‰ on δ²H‰
14 measurement^[37,38] Little information is available concerning the catalyst life time and its
15 regeneration. A lower efficiency of catalysts used in this study could have been the cause of
16 the large dispersion of deuterium enrichment measurement using equilibration. However the
17 enriched water samples from preliminary tests (Table 1) were measured using new platinum
18 catalysts with H₂O/H₂-equilibration method, and the standard deviations remain important in
19 the same way as standard deviations from samples of the nutritional intervention.
20
21
22
23
24
25
26
27
28
29
30
31
32

33 34 *Conclusion*

35 δ²H and δ¹⁸O in urine samples can be analysed using either equilibration or HTC-CF-IRMS.
36 Both methods were perfectly correlated and linearity of measurements was excellent in a
37 range of -55.5 ‰ to 220.7 ‰ for ¹⁸O, and of -428.0 ‰ to 1218.3 ‰ for ²H. Accuracy of
38 ²H- and ¹⁸O- measurements was acceptable for both techniques. Concerning high temperature
39 conversion, one disadvantage which is largely described in the literature is the memory
40 effect.^[27,34,32] With a regular maintenance of the reactor (every 2000 injections) and by taking
41 the various precautions described in the experimental section, this paper shows that it is
42 possible to obtain results with limited analytical variation and without any modification of the
43 high-temperature reactor.^[34] But this has a cost. Indeed consumables used to the maintenance
44 of the reactor are expensive. The volume of sample required with HTC method is reduced
45 compared to equilibration method. That can be a great advantage when urine samples have to
46 be collected in specific populations as new-born, or people with handicap (intellectual and/or
47 motor). Regarding the duration of the analyses (see Experimental part), time saving with HTC
48 method is real compared to equilibration method, provided that ²H and ¹⁸O enrichment
49 measurements are necessary for all samples analysed. Indeed, for a same number of samples
50 to measure, if only one isotope is needed, the duration of analyses is roughly equivalent.
51
52
53
54
55
56
57
58
59
60

Physiological results

Volume of total body water

Volumes of TBW were calculated from $\delta^{18}\text{O}\text{‰}$ enrichments measured either with the equilibration device or the HTC device using the equations (1) and (2) described in the experimental section. Individual results (Figure 3(A)) show differences of up to 2.2L and the results from 8 of 14 subjects show TBW differences less than or equal to 1L. The mean difference in the volume of TBW for each subject was $1.0\pm 0.7\text{L}$ (mean \pm SD) depending on the analytical method. Finally, for the 14 subjects, the volume of TBW calculated with the data obtained using equilibration or HTC were respectively $45.1\pm 1.0\text{L}$ and $45.7\pm 1.0\text{L}$ (mean \pm sem, Figure 3(B)). Thus, volume of TBW does not depend on the technique used for $\delta^{18}\text{O}$ enrichments. This was confirmed by applying a paired t-test ($p=0.0869$).

Dietary fatty acid oxidation

Figure 4 shows the 8h, 12h and 3 day cumulative percentage recoveries of d_{31} -palmitic acid in urine samples from the 14 subjects calculated with the data coming from the equilibration or from the HTC device. The calculation of palmitic acid oxidation (See equation (3), experimental section) required deuterium enrichment measurements in urine and the volume of total body water, obtained previously through $\delta^{18}\text{O}\text{‰}$ enrichment measurements. As shown in Figure 4(A), the recovery rate of deuterium in urine at 8h, 12h and 3 days post-dose were respectively $16.2\pm 1.6\%$ vs $16.2\pm 1.1\%$, $18.7\pm 2.0\%$ vs $17.6\pm 1.3\%$ and $21.7\pm 1.9\%$ vs $21.5\pm 1.3\%$ (mean \pm sem, data from equilibration vs HTC). A paired t-test showed no significant difference for d_{31} -palmitic acid recovery calculated either from the equilibration data or the HTC data, at 8h ($p=0.9715$), 12h ($p=0.2616$) and 3 days post-dose ($p=0.8840$). A Bland and Altman test (Fig.4(B)) shows differences between results from both methods as a function of the average of results obtained with each method. This diagram shows a mean bias of -0.14% according the analytical methods used, with a confidence interval between -6.39 to $+6.75\%$. Thus, both methods allow study of dietary lipid oxidation in man and generate similar results. Analytical variations remained lower than inter-subject variations.

CONCLUSIONS

A series of experiments conducted in this study indicated that $\delta^2\text{H}$ and $\delta^{18}\text{O}$ in urine samples can be analysed using either equilibration-CF-IRMS or HTC-CF-IRMS. Both methods were perfectly correlated, accuracy was acceptable and the linearity of enrichment

1
2
3 measurements was excellent for enrichments usually encountered in the field of human
4 nutrition. With the equilibration method, the dispersion of measurements is much greater than
5 when using HTC.
6
7

8 Applying these methods to the determination of d_{31} -palmitic acid oxidation resulted in
9 similar results and no significant difference was observed for fatty acid recovery and total
10 body water volume.
11

12 ^2H and ^{18}O enrichment measurements in biological fluids have numerous applications
13 in the field of nutrition. Indeed, measuring TBW also enables study of body composition;^[39]
14 ^2H and ^{18}O elimination rate calculation after doubly-labelled water ingestion allows for the
15 determination of total energy expenditure.^[3] Showing that these measurements are equivalent
16 using two commercially available devices based on fundamentally different principles is of
17 great interest.
18
19

20 Regarding the practical aspect of the two methods, due to the isotopic exchange
21 process, the equilibration method is expected to be less sensitive to impurities from biological
22 samples. However deuterium enrichment determination depends on the efficiency of the
23 catalyst. Large volumes of samples are required and the method is time-consuming because of
24 the necessity to analyse the biological samples for ^2H - and then ^{18}O - content. Conversely,
25 HTC gives ^2H - and ^{18}O - enrichment results in the same run.
26
27

28 Despite the drawbacks of the HTC method which include memory effects, limited
29 reactor lifetime and the cost of consumables, high temperature conversion analysis rather than
30 equilibration for measuring $\delta^2\text{H}$ and $\delta^{18}\text{O}$ enrichments in urines remains more convenient for
31 clinical studies where the number of samples for each subject is often high. However, it is
32 important to follow instructions to minimise inter-sample memory effects and special
33 attention should be paid to sample purification when analyses are performed using HTC. Even
34 if measured enrichments in biological samples are always compared to a basal value in
35 metabolic studies performed in the field of nutrition.
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Acknowledgements

We are indebted to all the staff of the Centre de Recherche en Nutrition Humaine Rhône-Alpes for their technical assistance in subject recruitment, sample collection and sample preparation. We also thank Dr Stéphane Blanc, Dr Julie-Anne Nazare and the anonymous reviewers for revising the manuscript and providing useful advice, as well as Lynn Richardson for language revision.

For Peer Review

REFERENCES

- [1] G.G. Dolnikowski, J.B. Marsh, S.K. Das, F.K. Welty. Stable isotopes in obesity research. *Mass Spectrom. Rev.* **2005**, *24*, 311.
- [2] D.A. Schoeller, E. van Santen, D.W. Peterson, W. Dietz, J. Jaspan, P.D. Klein. Total body water measurement in humans with ^{18}O and ^2H labeled water. *Am. J. Clin. Nutr.* **1980**, *33*, 2686.
- [3] D.A. Schoeller, E. Ravussin, Y. Schutz, K.J. Acheson, P. Baertschi, E. Jéquier. Energy expenditure by doubly labeled water: validation in humans and proposed calculation. *Am. J. Physiol.* **1986**, *250*, R823.
- [4] J.-P. Godin, A.-F. Mermoud, D. Rémond, M. Faure, D. Breuille, G. Williamson, E. Peré-Trepat, Z. Ramadan, L.-B. Fay, S. Kochhar. Simultaneous measurement of ^{13}C - and ^{15}N -isotopic enrichments of threonine by mass spectrometry. *Rapid Commun. Mass Spectrom.* **2009**, *23*, 1109.
- [5] T. Preston, A.C. Small. Improved measurement of protein synthesis in human subjects using ^2H -phenylalanine isotopomers and gas chromatography/mass spectrometry. *Rapid Commun. Mass Spectrom.* **2010**, *24*, 549.
- [6] V. Sauvinet, L. Gabert, D. Qin, C. Louche-Pélissier, M. Laville, M. Désage. Validation of pentaacetylaldonitrile derivative for dual ^2H gas chromatography/mass spectrometry and ^{13}C gas chromatography/combustion/isotope ratio mass spectrometry analysis of glucose. *Rapid Commun. Mass Spectrom.* **2009**, *23*, 3855.
- [7] J.-A. Nazare, A. de Rougemont, S. Normand, V. Sauvinet, M. Sothier, S. Vinoy, M. Désage, M. Laville. Effect of postprandial modulation of glucose availability: short- and long-term analysis. *Br. J. Nutr.* **2010**, *103*, 1461.
- [8] A. Bergouignan, G. Trudel, C. Simon, A. Chopard, D.A. Schoeller, I. Momken, S.B. Votruba, M. Desage, G.C. Burdge, G. Gauquelin-Koch, S. Normand, S. Blanc. Physical inactivity differentially alters dietary oleate and palmitate trafficking. *Diabetes* **2009**, *58*, 367.
- [9] L.S. Sidossis, A.R. Coggan, A. Gastaldelli, R.R. Wolfe. Pathway of free fatty acid oxidation in human subjects. Implications for tracer studies. *J. Clin. Invest.* **1995**, *95*, 278.
- [10] L.S. Sidossis, A.R. Coggan, A. Gastaldelli, R.R. Wolfe. A new correction factor for use in tracer estimations of plasma fatty acid oxidation. *Am. J. Physiol.* **1995**, *269*, E649.
- [11] S.B. Votruba, S.M. Zeddun, D.A. Schoeller. Validation of deuterium labeled fatty acids for the measurement of dietary fat oxidation: a method for measuring fat-oxidation in free-living subjects. *Int. J. Obes. Relat. Metab. Disord.* **2001**, *25*, 1240.
- [12] S.J. Prosser, C.M. Scrimgeour. High-precision determination of $^2\text{H}/^1\text{H}$ in H_2 and H_2O by continuous-flow isotope ratio mass spectrometry. *Anal. Chem.* **1995**, *67*, 1992.
- [13] D.C. McMillan, T. Preston, D.P. Taggart. Analysis of ^{18}O enrichment in biological fluids by continuous flow-isotope ratio mass spectrometry. *Biomed. Environ. Mass Spectrom.* **1989**, *18*, 543.
- [14] C. Huber, M. Leuenberger. Fast high-precision on-line determination of hydrogen isotope ratios of water or ice by continuous-flow isotope ratio mass spectrometry. *Rapid Commun. Mass Spectrom.* **2003**, *17*, 1319.
- [15] W.A. Brand, A.R. Tegtmeier, A. Hilker. Compound-specific isotope analysis: extending toward $^{15}\text{N}/^{14}\text{N}$ and $^{18}\text{O}/^{16}\text{O}$. *Org. Geochem.* **1994**, *21*, 585.
- [16] G.D. Farquhar, B.K. Henry, J.M. Styles. A rapid on-line technique for determination of oxygen isotope composition of nitrogen-containing organic matter and water. *Rapid Commun. Mass Spectrom.* **1997**, *11*, 1554.
- [17] J. Koziat. Isotope ratio mass spectrometric method for the on-line determination of oxygen-18 in organic matter. *J. Mass Spectrom.* **1997**, *32*, 103.
- [18] S. Epstein, T. Mayeda. Variation of O 18 content of waters from natural sources. *Geochim. Cosmochim. Acta* **1953**, *4*, 213.

- 1
2
3 [19] J.H. Rolston, J. Den Hartog, J.P. Butler. The deuterium isotope separation factor
4 between hydrogen and liquid water. *J. Phys. Chem.* **1976**, *80*, 1064.
- 5 [20] J. Horita, A. Ueda, K. Mizukami, I. Takatori. Automatic dD and d¹⁸O analyses of multi-
6 water samples using H₂- and CO₂-water equilibration methods with a common
7 equilibration set-up. *Appl. Radiat. Isot.* **1989**, *40*, 801.
- 8 [21] C. Bossu, B. Galusca, S. Normand, N. Germain, P. Collet, D. Frere, F. Lang, M.
9 Laville, B. Estour. Energy expenditure adjusted for body composition differentiates
10 constitutional thinness from both normal subjects and anorexia nervosa. *Am. J. Physiol. -*
11 *Endocrinology And Metabolism* **2007**, *292*, E132.
- 12 [22] D. Jacobi, A.-E. Perrin, N. Grosman, M.-F. Dore, S. Normand, J.-M. Oppert, C. Simon.
13 Physical Activity-Related Energy Expenditure With the RT3 and TriTrac
14 Accelerometers in Overweight Adults. *Obesity* **2007**, *15*, 950.
- 15 [23] M. Bonnefoy, M. Laville, R. Ecochard, J.-F. Jusot, S. Normand, S. Maillot, B. Lebreton,
16 M. Jauffret. Effects of branched amino acids supplementation in malnourished elderly
17 with catabolic status. *J. Nutr. Health Aging* **2010**, *14*, 579.
- 18 [24] T.B. Coplen, I.T. Harper. An improved technique for the ²H/¹H analysis of urines from
19 diabetic volunteers. *Biol. Mass Spectrom.* **1994**, *23*, 437.
- 20 [25] D.A. Schoeller, A.H. Luke. Rapid ¹⁸O analysis of CO₂ samples by continuous-flow
21 isotope ratio mass spectrometry. *J. Mass Spectrom.* **1997**, *32*, 1332.
- 22 [26] W.A. Brand, T.B. Coplen, A.T. Aerts-Bijma, J.K. Böhlke, M. Gehre, H. Geilmann, M.
23 Gröning, H.G. Jansen, H.A.J. Meijer, S.J. Mroczkowski, H. Qi, K. Soergel, H. Stuart-
24 Williams, S.M. Weise, R.A. Werner. Comprehensive inter-laboratory calibration of
25 reference materials for delta¹⁸O versus VSMOW using various on-line high-temperature
26 conversion techniques. *Rapid Commun. Mass Spectrom.* **2009**, *23*, 999.
- 27 [27] M. Richelle, C. Darimont, C. Piguet-Welsch, L.B. Fay. High-throughput simultaneous
28 determination of plasma water deuterium and 18-oxygen enrichment using a high-
29 temperature conversion elemental analyzer with isotope ratio mass spectrometry. *Rapid*
30 *Commun. Mass Spectrom.* **2004**, *18*, 795.
- 31 [28] N. Ripoche, V. Ferchaud-Roucher, M. Krempf, P. Ritz. D and ¹⁸O enrichment
32 measurements in biological fluids in a continuous-flow elemental analyser with an
33 isotope-ratio mass spectrometer using two configurations. *J Mass Spectrom.* **2006**, *41*,
34 1212.
- 35 [29] H. Schierbeek, R. Rieken, K.Y. Dorst, C. Penning, J.B. van Goudoever. Validation of
36 deuterium and oxygen18 in urine and saliva samples from children using on-line
37 continuous-flow isotope ratio mass spectrometry. *Rapid Commun. Mass Spectrom.* **2009**,
38 *23*, 3549.
- 39 [30] J. Horita. Hydrogen isotope analysis of natural waters using an H₂-water equilibration
40 method: A special implication to brines. *Chemical Geology: Isotope Geoscience section*
41 **1988**, *72*, 89.
- 42 [31] A.L. Sessions. Isotope-ratio detection for gas chromatography. *J. Sep. Sci.* **2006**, *29*,
43 1946.
- 44 [32] J. Olsen, I. Seierstad, B. Vinther, S. Johnsen, J. Heinemeier. Memory effect in
45 deuterium analysis by continuous flow isotope ratio measurement. *Int. J. Mass*
46 *Spectrom.* **2006**, *254*, 44.
- 47 [33] J. Morrison, T. Brockwell, T. Merren, F. Fourel, A.M. Phillips. On-Line High-Precision
48 Stable Hydrogen Isotopic Analyses on Nanoliter Water Samples. *Anal. Chem.* **2001**, *73*,
49 3570.
- 50 [34] M. Gehre, H. Geilmann, J. Richter, R.A. Werner, W.A. Brand. Continuous flow ²H/¹H
51 and ¹⁸O/¹⁶O analysis of water samples with dual inlet precision. *Rapid Commun. Mass*
52 *Spectrom.* **2004**, *18*, 2650.
- 53 [35] F.H. Lu. Online high-precision δ²H and δ¹⁸O analysis in water by pyrolysis. *Rapid*
54 *Commun. Mass Spectrom.* **2009**, *23*, 3144.
- 55
56
57
58
59
60

- 1
2
3 [36] J.M. Bland, D.G. Altman. Statistical methods for assessing agreement between two
4 methods of clinical measurement. *Lancet* **1986**, *1*, 307.
5 [37] J.T. Brenna, T.N. Corso, H.J. Tobias, R.J. Caimi. High-precision continuous-flow
6 isotope ratio mass spectrometry. *Mass Spectrom. Rev.* **1997**, *16*, 227.
7 [38] A.J. Midwood, B.A. McGaw. Recent developments in the analysis of light isotopes by
8 continuous flow isotope ratio mass spectrometry. *Anal. Commun.* **1999**, *36*, 291.
9 [39] N. Pace, E. Rathburn. Studies on body composition. III. The body water and chemically
10 combined nitrogen content in relation to fat content. *J. Biol. Chem.* **1945**, *158*, 685.
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

For Peer Review

Sample	$\delta^{18}\text{O} \pm \text{SD} (\text{‰})$						$\delta^2\text{H} \pm \text{SD} (\text{‰})$					
	CF-Equilibration			CF-HTC			CF-Equilibration			CF-HTC		
	Run1	Run2	Run3	Run1	Run2	Run3	Run1	Run2	Run3	Run1	Run2	Run3
SLAP2	-55.46 <i>0.38</i>	-55.30 <i>0.28</i>	-55.04 <i>0.34</i>	-55.24 <i>0.14</i>	-54.96 <i>0.20</i>	-55.02 <i>0.13</i>	-428.32 <i>6.83</i>	-433.52 <i>5.88</i>	-429.22 <i>7.07</i>	-420.93 <i>0.40</i>	-423.90 <i>0.28</i>	-419.96 <i>0.33</i>
GISP	-24.74 <i>0.33</i>	-24.71 <i>0.29</i>	-24.62 <i>0.29</i>	-24.81 <i>0.21</i>	-24.86 <i>0.25</i>	-25.06 <i>0.21</i>	-191.77 <i>5.19</i>	-190.91 <i>8.59</i>	-191.43 <i>6.02</i>	-187.06 <i>0.13</i>	-188.42 <i>0.20</i>	-186.76 <i>0.35</i>
H2O 1	-7.67 <i>0.30</i>	-7.75 <i>0.24</i>	-7.79 <i>0.27</i>	-7.75 <i>0.18</i>	-8.26 <i>0.36</i>	-8.33 <i>0.27</i>	-64.32 <i>6.81</i>	-64.14 <i>5.17</i>	-65.65 <i>6.87</i>	-62.21 <i>0.31</i>	-63.08 <i>0.28</i>	-62.18 <i>0.15</i>
H2O 2	-4.55 <i>0.32</i>	-4.63 <i>0.27</i>	-4.63 <i>0.27</i>	-4.59 <i>0.08</i>	-4.99 <i>0.15</i>	-5.24 <i>0.18</i>	-21.74 <i>6.91</i>	-20.94 <i>5.60</i>	-16.98 <i>7.19</i>	-20.70 <i>0.13</i>	-21.19 <i>0.28</i>	-20.75 <i>0.22</i>
VSMOW2	-0.01 <i>0.33</i>	-0.06 <i>0.27</i>	-0.02 <i>0.28</i>	0.42 <i>0.06</i>	0.93 <i>0.30</i>	1.76 <i>0.15</i>	0.77 <i>7.64</i>	-3.04 <i>5.84</i>	-2.19 <i>8.58</i>	1.18 <i>0.30</i>	1.46 <i>0.20</i>	1.73 <i>0.29</i>
H2O 3	1.67 <i>0.28</i>	1.54 <i>0.30</i>	1.50 <i>0.25</i>	1.30 <i>0.39</i>	1.34 <i>0.22</i>	1.27 <i>0.08</i>	20.72 <i>5.13</i>	18.27 <i>9.75</i>	17.18 <i>9.09</i>	18.15 <i>0.24</i>	17.60 <i>0.19</i>	18.24 <i>0.18</i>
H2O 4	13.71 <i>0.30</i>	13.29 <i>0.28</i>	12.97 <i>0.30</i>	12.80 <i>0.26</i>	13.67 <i>0.35</i>	13.18 <i>0.39</i>	66.50 <i>8.85</i>	59.35 <i>6.46</i>	66.45 <i>8.80</i>	62.36 <i>0.17</i>	61.94 <i>0.19</i>	62.07 <i>0.48</i>
H2O 5	28.97 <i>0.28</i>	28.58 <i>0.20</i>	28.65 <i>0.26</i>	28.43 <i>0.10</i>	28.74 <i>0.23</i>	28.37 <i>0.30</i>	199.00 <i>6.66</i>	195.59 <i>7.03</i>	197.55 <i>6.25</i>	195.17 <i>0.21</i>	194.90 <i>0.34</i>	195.04 <i>0.28</i>
H2O 6	48.75 <i>0.24</i>	48.48 <i>0.22</i>	48.65 <i>0.23</i>	48.68 <i>0.15</i>	48.55 <i>0.26</i>	48.00 <i>0.23</i>	473.83 <i>5.09</i>	472.64 <i>7.03</i>	472.00 <i>6.19</i>	470.19 <i>0.30</i>	470.11 <i>0.33</i>	469.80 <i>0.56</i>
H2O 7	102.79 <i>0.14</i>	102.50 <i>0.14</i>	102.37 <i>0.20</i>	102.30 <i>0.36</i>	102.41 <i>0.10</i>	101.92 <i>0.27</i>	826.26 <i>5.23</i>	827.74 <i>8.34</i>	825.35 <i>8.40</i>	824.78 <i>0.51</i>	825.74 <i>0.26</i>	824.85 <i>0.65</i>
H2O 8	220.91 <i>0.11</i>	221.10 <i>0.20</i>	221.86 <i>0.67</i>	220.73 <i>0.54</i>	220.37 <i>0.46</i>	220.52 <i>0.31</i>	1215.08 <i>7.46</i>	1211.59 <i>7.26</i>	1213.82 <i>5.70</i>	1211.55 <i>0.63</i>	1212.51 <i>0.50</i>	1210.62 <i>0.77</i>
Urine 1	-2.39 <i>0.20</i>	-2.52 <i>0.27</i>	-2.41 <i>0.19</i>	-3.22 <i>0.05</i>	-3.07 <i>0.09</i>	-3.03 <i>0.08</i>	-26.21 <i>8.06</i>	-30.32 <i>10.37</i>	-30.56 <i>11.12</i>	-31.12 <i>1.04</i>	-31.74 <i>0.39</i>	-31.44 <i>0.53</i>
Urine 2	0.24 <i>0.27</i>	-0.04 <i>0.15</i>	0.03 <i>0.12</i>	-0.60 <i>0.03</i>	-0.57 <i>0.02</i>	-0.63 <i>0.10</i>	-2.43 <i>6.31</i>	-1.29 <i>4.73</i>	-8.48 <i>13.31</i>	-10.23 <i>0.12</i>	-9.68 <i>1.31</i>	-10.73 <i>0.29</i>
Urine 3	2.40 <i>0.22</i>	2.42 <i>0.22</i>	2.31 <i>0.12</i>	1.74 <i>0.03</i>	1.76 <i>0.04</i>	1.71 <i>0.08</i>	29.75 <i>7.51</i>	29.20 <i>9.65</i>	32.00 <i>9.17</i>	20.79 <i>0.29</i>	20.45 <i>0.12</i>	20.72 <i>0.66</i>
Urine 4	9.93 <i>0.26</i>	9.79 <i>0.26</i>	9.81 <i>0.16</i>	9.12 <i>0.06</i>	9.22 <i>0.05</i>	9.13 <i>0.03</i>	59.20 <i>12.30</i>	59.81 <i>6.36</i>	60.35 <i>6.53</i>	50.82 <i>0.38</i>	49.69 <i>0.34</i>	49.86 <i>0.28</i>
Urine 5	14.98 <i>0.21</i>	14.72 <i>0.23</i>	14.56 <i>0.14</i>	14.03 <i>0.07</i>	14.12 <i>0.07</i>	14.04 <i>0.08</i>	81.77 <i>12.70</i>	85.49 <i>5.55</i>	87.74 <i>5.22</i>	76.37 <i>0.81</i>	76.62 <i>0.47</i>	77.07 <i>0.16</i>
Urine 6	21.95 <i>0.20</i>	21.72 <i>0.20</i>	21.62 <i>0.13</i>	20.92 <i>0.03</i>	20.95 <i>0.06</i>	20.87 <i>0.06</i>	167.57 <i>7.36</i>	160.77 <i>3.88</i>	155.79 <i>9.88</i>	149.57 <i>0.40</i>	150.04 <i>0.45</i>	149.99 <i>0.53</i>
Urine 7	38.78 <i>0.19</i>	38.47 <i>0.18</i>	38.12 <i>0.14</i>	37.62 <i>0.04</i>	37.65 <i>0.14</i>	37.67 <i>0.05</i>	506.40 <i>10.29</i>	507.45 <i>6.93</i>	513.99 <i>14.78</i>	501.09 <i>0.79</i>	503.90 <i>1.10</i>	502.59 <i>0.97</i>
Urine 8	122.22 <i>0.08</i>	121.98 <i>0.09</i>	121.39 <i>0.16</i>	121.14 <i>0.06</i>	121.25 <i>0.03</i>	121.17 <i>0.06</i>	915.63 <i>9.48</i>	916.79 <i>5.86</i>	918.35 <i>7.18</i>	908.84 <i>0.23</i>	908.62 <i>1.77</i>	911.34 <i>1.56</i>
Urine 9	201.59 <i>0.09</i>	200.77 <i>0.08</i>	200.15 <i>0.13</i>	200.01 <i>0.05</i>	200.36 <i>0.08</i>	200.54 <i>0.10</i>	1817.11 <i>4.83</i>	1816.85 <i>12.12</i>	1812.68 <i>8.73</i>	1814.03 <i>1.41</i>	1818.50 <i>1.03</i>	1824.60 <i>0.83</i>

Table 1. ^{18}O - and ^2H - enrichments measured either by CF-equilibration or CF-HTC in enriched water samples including reference waters from IAEA (SLAP2, GISP and VSMOW2) and in enriched urine samples. Data were normalized against calibration points supplied by Iso-analytical Limited (IA R053, IA R054 and IA R055). Results are presented as the mean (in bold) \pm standard deviation (SD, in italic). The injection conditions are described in the experimental section for each method (paragraphs “Continuous Flow Equilibration” and “Continuous Flow High Temperature Conversion”). Measurements were done in 3 batches of analyses performed on 3 different days using both techniques (Run1, Run 2 and Run 3).

	¹⁸ O						² H						
	CF-Equilibration			CF-HTC			CF-Equilibration			CF-HTC			
	Slope	Intercept	R ²	Slope	Intercept	R ²	Slope	Intercept	R ²	Slope	Intercept	R ²	
H ₂ O	Run 1	1.0009	0.5598	1.0000	0.9997	0.4017	1.0000	0.9991	2.1431	1.0000	0.9939	2.8098	1.0000
	Run 2	1.0011	0.4322	1.0000	0.9982	0.5057	1.0000	0.9999	-0.1234	0.9999	0.9958	2.0114	1.0000
	Run 3	1.0032	0.4498	1.0000	0.9981	0.3658	0.9999	0.9985	1.4399	0.9999	0.9931	2.9819	1.0000
	Mean	1.0017	0.4806	1.0000	0.9987	0.4244	1.0000	0.9992	1.1532	0.9999	0.9943	2.6010	1.0000
	<i>SD</i>	<i>0.0013</i>	<i>0.0692</i>	<i>1.3E-05</i>	<i>0.0009</i>	<i>0.0726</i>	<i>1.9E-05</i>	<i>0.0007</i>	<i>1.1601</i>	<i>8.8E-06</i>	<i>0.0014</i>	<i>0.5178</i>	<i>1.5E-06</i>

Table 2. Regression parameters calculated from expected delta values (X-axis, Table 3) and ¹⁸O- and ²H- enrichments from enriched waters measured either by CF-equilibration or CF-HTC (Y-axis, Table 1). Isotopic enrichments ranged from -55.5 ‰ to +220.78 ‰ for ¹⁸O and from -428 ‰ to +1418 ‰ for ²H relative to VSMOW. Results are presented as the mean (in bold) ± standard deviation (SD, in italic) of the 3 batches of analyses (Run 1, Run 2 and Run 3).

Accuracy ($\delta\%$)		Expected ($\delta\%$)	CF-Equilibration			CF-HTC		
			Run 1	Run 2	Run 3	Run 1	Run 2	Run 3
^{18}O	SLAP2	-55.5	-0.04	-0.20	-0.46	-0.26	-0.54	-0.48
	GISP	-24.8	-0.06	-0.09	-0.18	0.01	0.06	0.26
	H2O 1	-8.2	-0.57	-0.49	-0.45	-0.49	0.02	0.09
	H2O 2	-5.3	-0.70	-0.62	-0.62	-0.66	-0.26	-0.01
	VSMOW2	0.0	0.01	0.06	0.02	-0.42	-0.93	-1.76
	H2O 3	1.0	-0.69	-0.56	-0.52	-0.32	-0.36	-0.29
	H2O 4	12.5	-1.17	-0.75	-0.43	-0.17	-1.04	-0.55
	H2O 5	27.9	-1.08	-0.69	-0.76	-0.54	-0.85	-0.48
	H2O 6	47.8	-0.97	-0.70	-0.87	-0.90	-0.77	-0.22
	H2O 7	101.8	-1.01	-0.72	-0.59	-0.52	-0.63	-0.14
H2O 8	220.7	-0.24	-0.43	-1.19	-0.06	0.30	0.15	
Mean \pm SD			-0.54 \pm 0.30			-0.39 \pm 0.34		
^2H	SLAP2	-428.0	0.32	5.52	1.22	-7.07	-4.10	-8.04
	GISP	-189.5	2.27	1.41	1.93	-2.44	-1.08	-2.74
	H2O 1	-65.2	-0.91	-1.09	0.42	-3.02	-2.15	-3.05
	H2O 2	-23.9	-2.17	-2.97	-6.93	-3.21	-2.72	-3.16
	VSMOW2	0.0	-0.77	3.04	2.19	-1.18	-1.46	-1.73
	H2O 3	16.2	-4.48	-2.03	-0.94	-1.91	-1.36	-2.00
	H2O 4	58.0	-8.51	-1.36	-8.46	-4.37	-3.95	-4.08
	H2O 5	194.2	-4.83	-1.42	-3.38	-1.00	-0.73	-0.87
	H2O 6	471.7	-2.15	-0.96	-0.32	1.49	1.57	1.88
	H2O 7	822.5	-3.80	-5.28	-2.89	-2.32	-3.28	-2.39
H2O 8	1218.3	3.22	6.71	4.48	6.75	5.79	7.68	
Mean \pm SD			-1.00 \pm 3.33			-1.52 \pm 3.39		

Table 3. Accuracy (difference between the expected value and the measured value in ‰) of ^2H - and ^{18}O - measurements in water using either CF-Equilibration or CF-HTC. Accuracy results were calculated from data presented in Table 1. Three batches of analyses were performed on 3 different days using both techniques (Run 1, Run 2 and Run 3).

Correlation parameters		^{18}O	^2H
H ₂ O	Slope	1.0030	1.0049
	Intercept	0.0558	-1.4604
	R	1.0000	1.0000
Urine	Slope	0.9993	0.9948
	Intercept	0.7228	8.4954
	R	1.0000	1.0000

Table 4. Correlation between $\delta^{18}\text{O}$ - and $\delta^2\text{H}$ - measurements obtained from CF-Equilibration (Y-axis) and CF-HTC (X-axis) techniques. The correlation parameters were calculated from data presented in Table 1. The samples were enriched and non-enriched waters (including reference waters from IAEA, SLAP2, GISP and VSMOW2) or ^{18}O - and ^2H - enriched urines. All were measured in 3 batches of analyses performed on 3 different days using both techniques. Injection conditions are described in the experimental section.

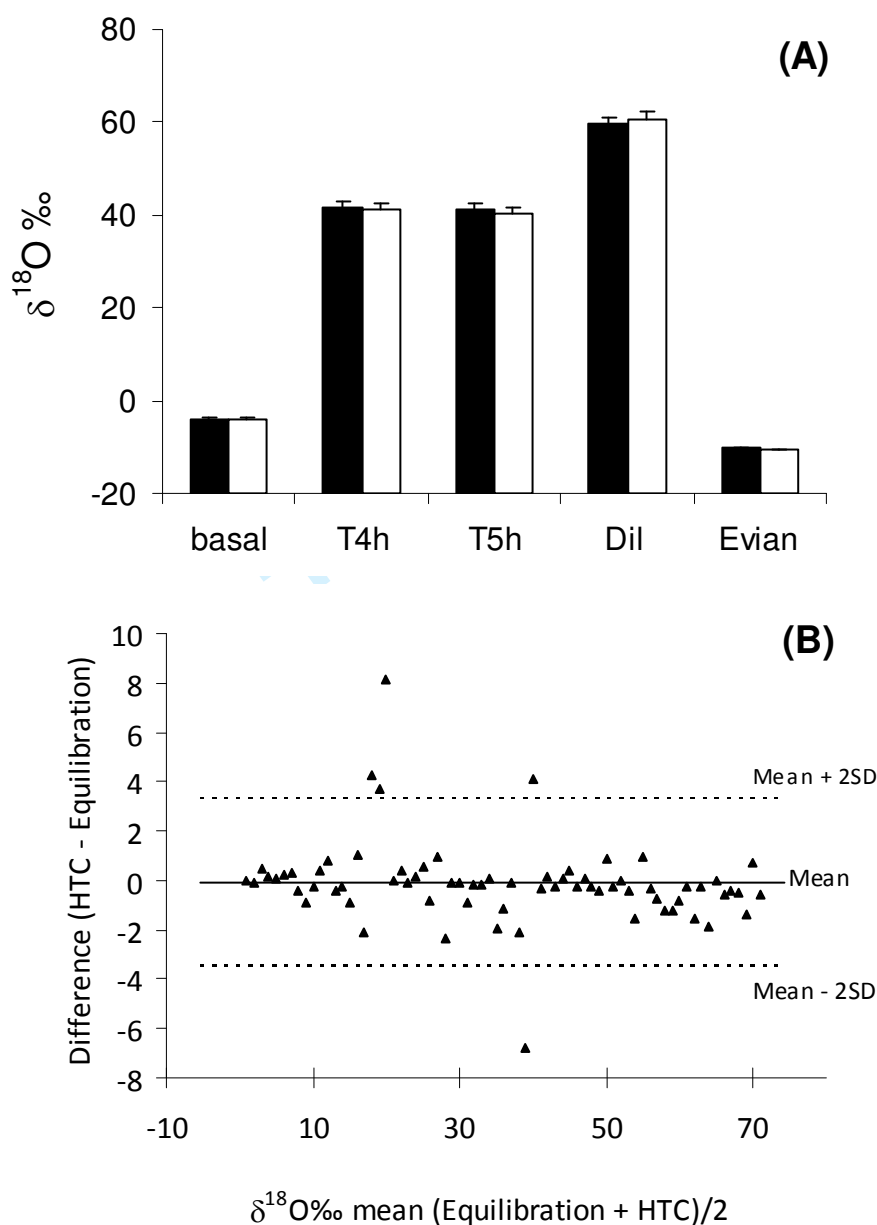


Figure 1. $\delta^{18}\text{O}\text{‰}$ enrichments in urine (basal, T4h and T5h) after ingestion of H_2^{18}O ($0.5\text{g}\cdot\text{kg}^{-1}$, $10\%^{18}\text{O}$), and in the dilution of the ingested H_2^{18}O dose in Evian water (Dil.) (Fig.2(A)).

Data are presented as the mean values ($\pm\text{sem}$) for samples of 14 subjects measured by continuous flow IRMS coupled to either an equilibration device (■) or a HTC device (□). A Bland and Altman test (Fig.2(B)) shows differences between results from both methods as a function of the average of results obtained with each method. This diagram shows a mean bias of 0.119‰ between the two methods, with a confidence interval between -3.51 and $+3.27\text{‰}$.

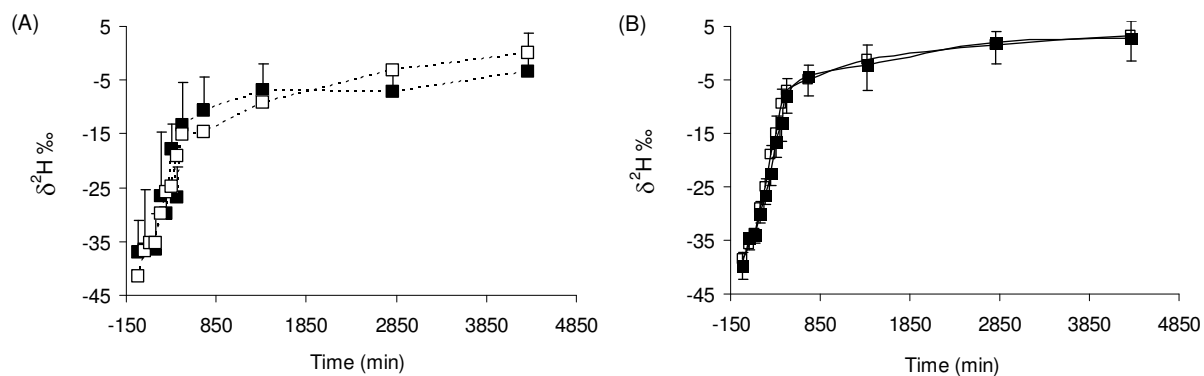


Figure 2. $\delta^2\text{H}\text{‰}$ evolution in urine until 3 days after ingestion of d_{31} -palmitic acid ($20\text{mg}\cdot\text{kg}^{-1}$) measured by continuous flow IRMS coupled either to an equilibration device (■) or a HTC device (□). Data are presented as the mean of injections ($\pm\text{SD}$) for 1 subject (A) and as the mean values ($\pm\text{sem}$) for 14 subjects (B). A mixed model showed no difference for the $\delta^2\text{H}\text{‰}$ measurement between the two methods used ($p=0.513$).

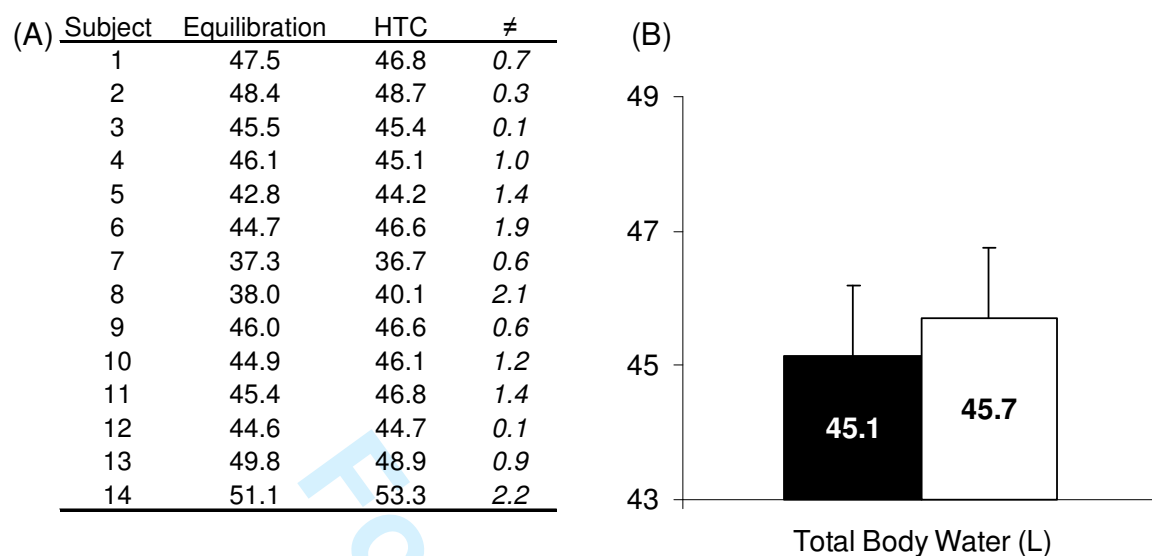


Figure 3. Total body water in L calculated from $\delta^{18}\text{O}\%$ enrichments measured either with equilibration (■) or HTC (□) techniques, using equations (1) and (2) (See experimental section). Individual results and differences (\neq) between values for the 14 subjects are presented (A) and the average \pm sem (B). No significant difference in volumes of Total Body Water depending on the analytical method was revealed (paired t-test, $p=0.0869$).

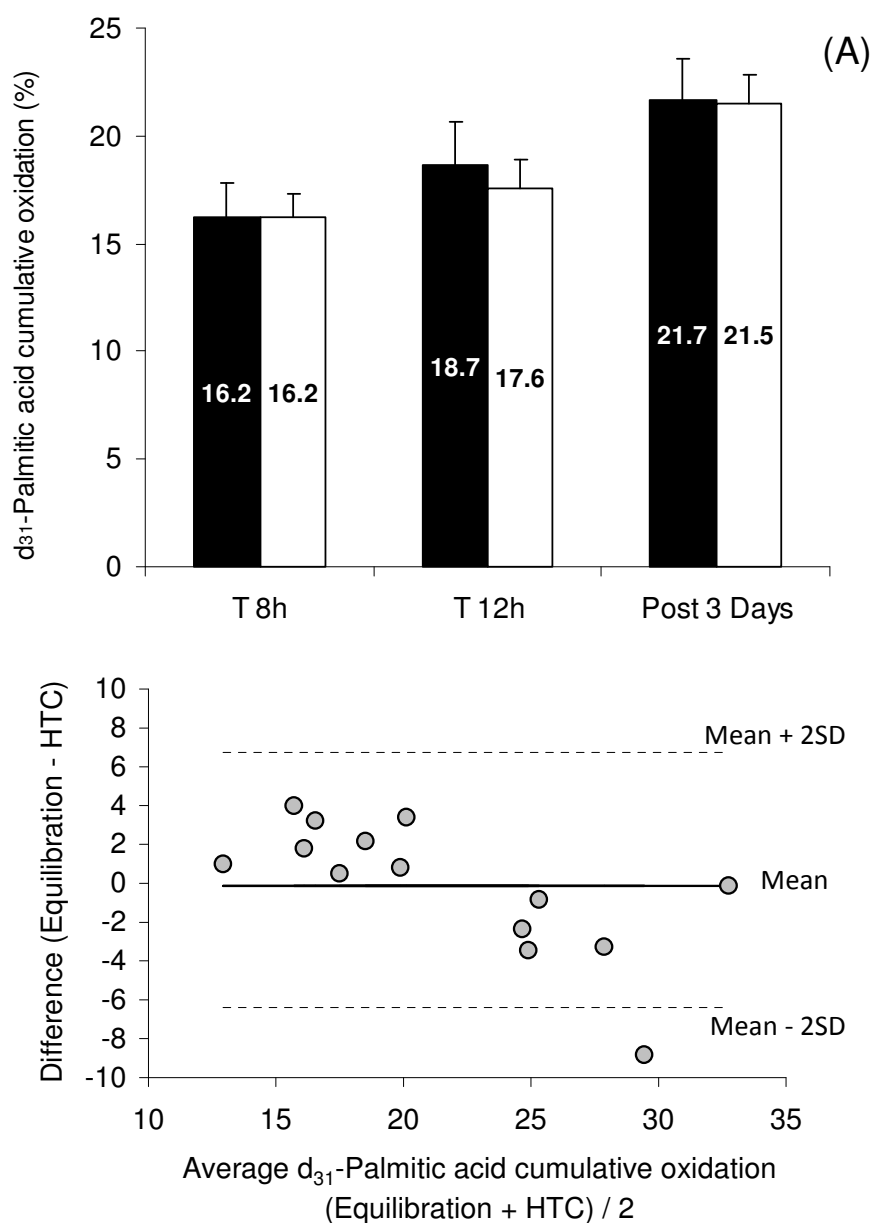


Figure 4. Cumulative recoveries expressed in % (mean \pm sem) of d₃₁-palmitic acid until 3 days post-ingestion (Fig.4(A)), were calculated from $\delta^{2}\text{H}\%$ enrichment measurements and TBW obtained either from equilibration (■) or HTC (□) techniques, using equation (3) (See experimental section). Data are presented as the mean values (\pm sem) obtained from the samples of 14 subjects. A paired t-test showed no significant difference for d₃₁-palmitic acid recovery calculated either from equilibration data or HTC data, at T 8h ($p= 0.9715$), T 12h ($p= 0.2616$) and 3 days post-dose ($p= 0.8840$). A Bland and Altman test (Fig.4(B)) shows differences between results from both methods as a function of the average of results obtained with each method. This diagram shows a mean bias of -0.14% according the analytical methods used, with a confidence interval between -6.39 to $+6.75\%$.